
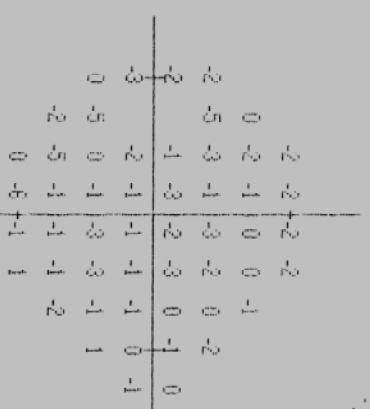
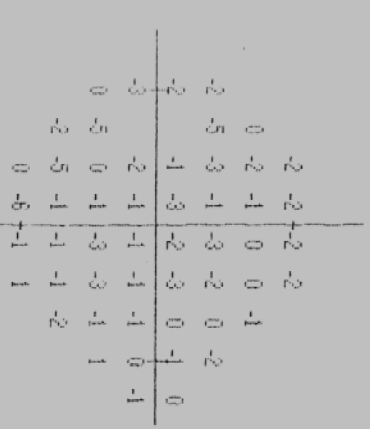


Ocular Refill 24 - 22
 KISTER, CHAD
 THRESHOLD TEST
 PATIENTS III, WHITE, BROWN 31.5 OSB BLIND SPOT CHECK SIZE III
 STRATEGY FULL THRESHOLD
 FRSTPRAC

BIRTHDATE 07-20-70 DATE 12-23-92 TIME 10:11:46 AM
 FIXATION TARGET CENTRAL IO PUPIL DIAMETER 6.0
 RX USED + 0.00 OS OX OS PUPIL DIAMETER 6.0
 VA

B.M. Kelly

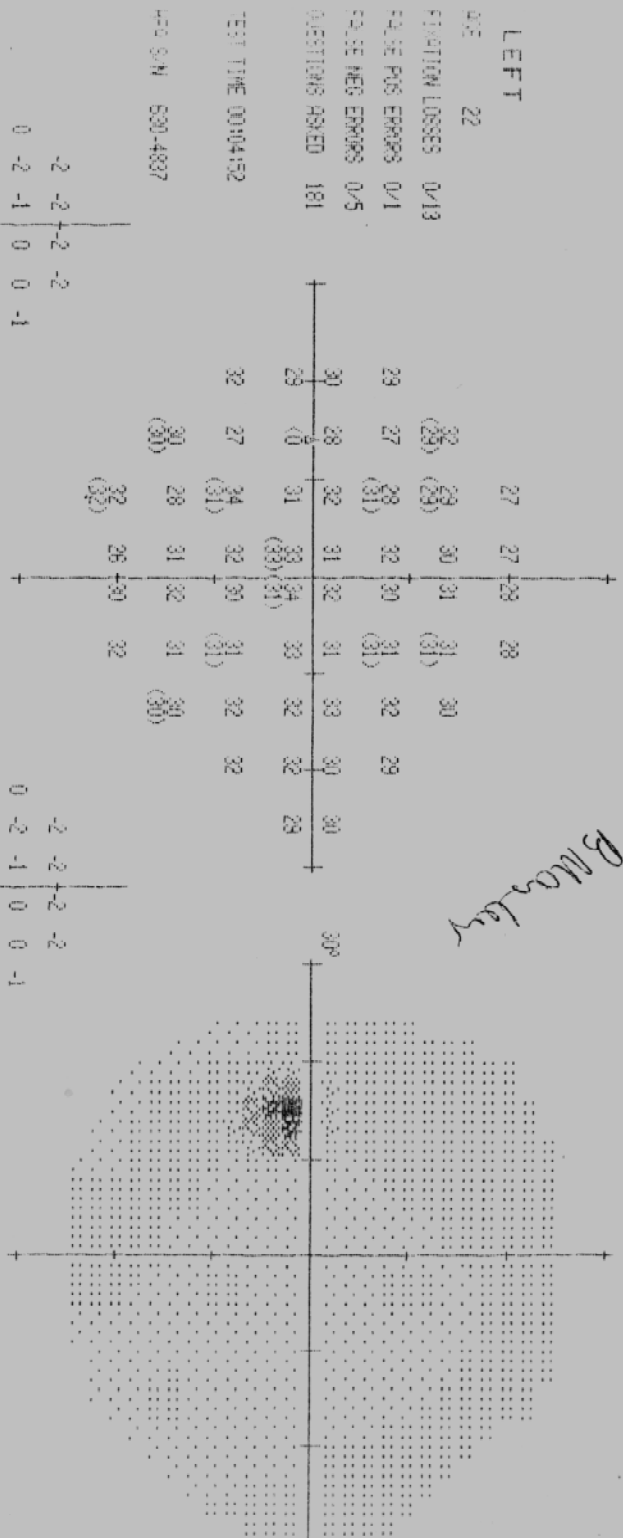

MD -1.45 08
 PSD 1.39 08
 SF 1.17 08
 PRSD 0.62 08

PROBABILITY SYMBOLS
 :: P < 5%
 < P < 2%
 < P < 1%
 ■ P < 0.5%

SYM	OSB	IRB	GRAYTONE SYMBOLS	REV BD
.8	2.5	8	25	79
.1	1	3.2	10	32
41	36	31	26	21
50	40	35	30	25
			20	16
			15	11
			10	6
			5	1
				50

COLUMBUS OPHTHALMOLOGY
 ORLANDO, LOTHES, BERAN
 6350 FRANTZ ROAD
 DUBLIN, OHIO 43017
 614/766-2008
 HUMPHREY INSTRUMENTS
 A CARL ZEISS COMPANY